


## Emergence width options

The functional and esthetic outcome achieved with Atlantis abutments is a result of the size of the healing space, the emergence width option selected and the position of the restorative margin.

**Note:** The default emergence width option for Atlantis abutments is contour tissue.

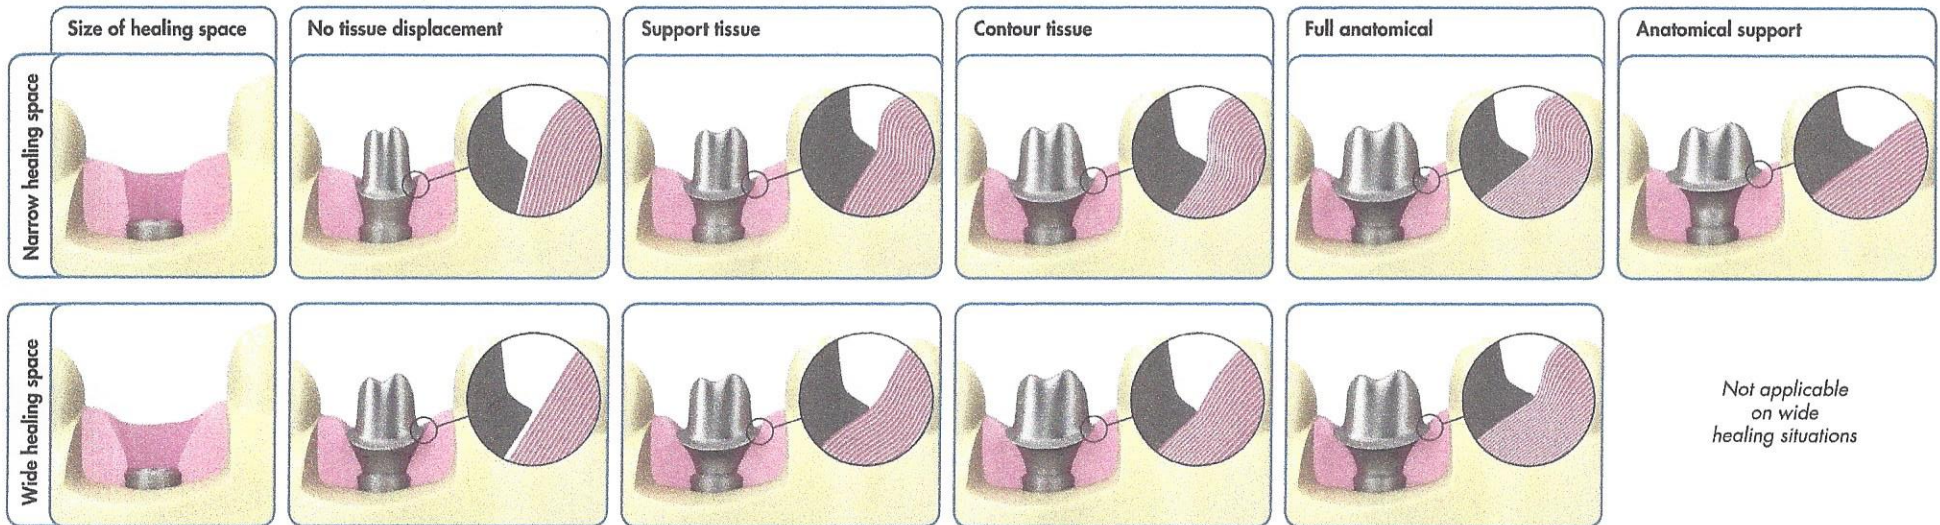

### 1. No tissue displacement

Smallest diameter, nonanatomically shaped abutment with no soft tissue support. The abutment will not touch the soft tissue.

### 2. Support tissue

Anatomically shaped abutment will be up to 0.2 mm larger than sulcus of silicone model of soft tissue provided with desired emergence profile. "Easy" insertion.

### 3. Contour tissue

Medium diameter anatomically shaped abutment up to 1.0 mm larger than sulcus of model of soft tissue provided.

### 4. Full anatomical

Largest diameter abutment provided with best emergence profile possible. A surgical incision for placement may be required.

### 5. Anatomical support

Ideal for narrow healing space compared to the edentulous situation in the "non-esthetic" zone. The size of the abutment will be anatomically adapted, the margins will be at gingiva level and the emergence shape will be as concave as possible.